

# **Crystal Digital PCR® Assay**

#### Information Sheet

For Research Use Only. Not for use in diagnostic procedures.

#### **Product Name**

EGFR (drop-off Del19) Crystal Digital PCR® Assay (R51026)

#### **Description**

Targets	Sample Type	<b>Detection Channels</b>	Multiplex
EGFR (drop-off Del19)	DNA	Blue/Green	2

The EGFR (drop-off Del19) Crystal Digital PCR® Assay is a 10X assay designed to detect and quantify EGFR Exon 19 deletion mutations using the Ruby Chip and based on the drop-off approach (refer to the technical note "Quantify Drop-off for digital PCR assays with Crystal Miner", <a href="https://www.stillatechnologies.com/">https://www.stillatechnologies.com/</a>). EGFR encodes for the epidermal growth factor receptor, a protein that plays a crucial role in cell growth, proliferation, and differentiation. This assay is available in 200 and 1000 reaction formats.

#### **Assay configuration**

The table below indicates with a "X" which channel(s) are used for each target in the assay:

Targets	Blue	Teal	Green	Yellow	Red	Infra-Red	Long-Shift
Wild-type (WT) EGFR ex19	X		X				
EGFR del19 (between I744 and E749)			X				
EGFR del19 (between K754 and L760)	Х						

#### Components

EGFR (drop-off del19) Crystal Digital PCR® Assay comprises two reagents: a pool of the assay specific primers and Crystal Flex Probes and a Positive Control. Please refer to the lot specific Certificate of Conformity for characterized concentration, available for download at the Technical Resources section of the Stilla Technologies website.

Component Name	Reference	Concentration	Description
EGFR (drop-off Del19) Crystal Digital PCR® Assay	R51026	10X	Detects deletions between codons I744 and L769 in the exon 19 of EGFR gene
EGFR Positive Control	R51025.PC0	10X	Contains: hgDNA, Synthetic EGFR mutants (E746-A750del, L858R, L861Q, T790M, C797S)

## **Thermocycling Programs**

#### On the naica® system:

Step		Ramp rate
Step 1	Partition for Ruby Chip	-
Step 2	Temperature 95°C for 180 seconds	1°C/sec
Step 3	Begin Loop for 60 Iterations	-
Step 3.1	Temperature 95°C for 15 seconds	1°C/sec
Step 3.2	Temperature 58°C for 30 seconds	1°C/sec
Step 4	Release for Ruby Chip	-

#### On the Nio™ Digital PCR:

Step		Ramp rate
Step 1	Partition for Ruby Chip	-
Step 2	Temperature 95°C for 180 seconds	1°C/sec
Step 3	Begin Loop for 60 Iterations	-
Step 3.1	Temperature 95°C for 15 seconds	2°C/sec
Step 3.2	Temperature 60°C for 30 seconds	2°C/sec
Step 4	Step 4 Temperature 58°C for 300 seconds	
Step 5	Release for Ruby Chip	-

# **Image Acquisition**

Download the dedicated scanning file from the Technical Resources section of the Stilla Technologies website:

- ScanningTemplate\_Prism3\_EGFR\_R51026.ncx (3-color naica® system)
- ScanningTemplate\_Prism6\_EGFR\_R51026.ncx (6-color naica® system)
- NioProtocol\_3C-60X-60°C-30s.nioprotocol (Nio™ Digital PCR)
- NioAssay\_3C\_EGFR\_R51026.nioassay (Nio™ Digital PCR)

## **Image Analysis**

The following files are embedded in the dedicated scanning files listed above:

- CompensationMatrix\_Prism3\_EGFR\_R51026.ncm (3-color naica® system)
- UniversalCompMatrix\_3C\_Prism6-Nio.ncm (6-color naica® system, Nio™ Digital PCR)
- AnalysisConfiguration\_Prism3\_EGFR\_R51026\_Polygons.nca (3-color naica® system)
- AnalysisConfiguration\_Prism6\_EGFR\_R51026\_Polygons.nca (6-color naica® system)
- AnalysisConfiguration\_Nio\_EGFR\_R51026\_Polygons.nca (Nio™ Digital PCR)

## **Consumables Required but Not Provided**

- Ruby Chip (C16011)
- naica® PCR MIX 10X (R10106)
- Crystal Universal Reporters 3 (R41401 200 reactions, R41402 1000 reactions)
- Nuclease-free water

### **Instruction for PCR Mix Preparation**

Specific instructions for preparing the PCR mix are given below.

Reagent Name	Initial Concentrat	ion Final Concentration	Volume per reaction (µL)
naica® PCR MIX Buffer A	10x	1x	0.60
naica® PCR MIX Buffer B	100%	4%	0.24
Crystal Digital PCR® Assay	10x	1x	0.60
Crystal Universal Reporter Tube A	40x	1x	0.15
Nuclease-free water	NA	NA	Variable
Template DNA	NA	NA	Variable
or Positive Control O	10x	1x	0.60
Total reaction volume (μL)			6.0

# **Representative Data and Instructions for Analysis**

In the menu "Analyze data, Plots & Populations", view the results in 2D dot plot. Check or manually adjust the position of the polygons for each target population according to the Positive Control. If needed, select "individual per chamber" in the thresholding mode to adjust the polygons for each sample. Examples of results obtained on the Nio™+ are given below.

Wet lab testing was carried out using genomic hgDNA as a negative control and a positive control consisting of hgDNA and synthetic EGFR mutants (E746-A750del, L858R, L861Q, T790M, C797S). Synthetic EGFR mutant was also tested individually (E746-A750del).



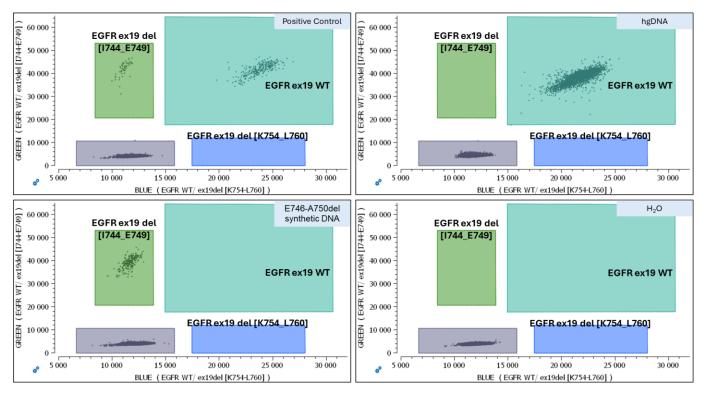


Figure 1: 2D plots obtained during wet lab testing on the Nio™+. The polygons should be adjusted for each target population and for each sample.



Registered names and trademarks used in this document, even when not specifically marked, are not to be considered unprotected by law.

