

# Crystal Digital PCR® Assay

## Information Sheet

For Research Use Only. Not for use in diagnostic procedures.

### Product Name

TERT (Reference, SLC12A7, TSN, C228T, C242T-243T, C250T) Crystal Digital PCR® Assay (R51024)

### Description

#### Detected Targets

Targets	Sample Type	Detection Channels	Multiplex
TERT Reference, SLC12A7, TSN, C228T, C242T-243T, C250T	DNA	Blue/Teal/Green/ Yellow/Red/Infra-Red	6

TERT (Reference/SLC12A7/228T/C242T-C243T/C250T/TSN) Crystal Digital PCR® Assay is a 10X assay designed to detect and quantify 3 mutations in the TERT promoter using the Ruby Chip. Three references are detected and used to quantify TERT gene amplification: a reference on the TERT gene, a reference on a gene located on the same chromosome as TERT (SLC12A7) and a reference on a different chromosome (TSN). TERT plays a critical role in cellular mechanisms linked to cancer progression, notably in maintaining telomere length and promoting immortalization.

#### Multiplexing Strategy: Color-Combination

This assay relies on the Color-Combination multiplexing strategy proprietary to Stilla Technologies, in which each target is detected, differentiated, and quantified by Crystal Digital PCR® using 2 fluorophores.

The table below indicates with a "X" which channel(s) are used for each target in the assay:

Targets	Base changes	Blue	Teal	Green	Yellow	Red	Infra-Red	Long-Shift
Reference (REF) TERT	N/A	X						
SLC12A7	N/A		X					
TSN	N/A						X	
TERT C228T	c.-124C > T	X		X				
TERT C242T-C243T	c.-138/c.-139 C > T	X			X			
TERT C250T	c.-146C > T	X				X		

## Components

TERT (Reference, SLC12A7, TSN, C228T, C242T-243T, C250T) Crystal Digital PCR® Assay comprises two reagents: a pool of the assay specific primers and Crystal Flex Probes and a Positive Control. Please refer to the lot specific Certificate of Conformity for characterized concentration, available for download at the Technical Resources section of the Stilla Technologies website.

Component Name	Reference	Concentration	Description
<b>TERT (Reference/ SLC12A7/228T/C242T-C243T /C250T/TSN) Crystal Digital PCR® Assay</b>	R51024	10X	Detects 3 mutations in the TERT promoter
<b>TERT Positive Control</b>	R51024.PC0	10X	Contains: hgDNA, Synthetic TERT mutants (C228T, C242T-C243T, C250T)

## Thermocycling Programs

### On the naica® system:

Step		Ramp rate
<b>Step 1</b>	Partition for Ruby Chip	-
<b>Step 2</b>	Temperature 95°C for 180 seconds	1°C/sec
<b>Step 3</b>	Begin Loop for 60 Iterations	-
<b>Step 3.1</b>	Temperature 95°C for 15 seconds	1°C/sec
<b>Step 3.2</b>	Temperature 62°C for 60 seconds	1°C/sec
<b>Step 4</b>	Temperature 58°C for 300 seconds	1°C/sec
<b>Step 5</b>	Release for Ruby Chip	-

### On the Nio™ Digital PCR:

Step		Ramp rate
<b>Step 1</b>	Partition for Ruby Chip	-
<b>Step 2</b>	Temperature 95°C for 180 seconds	1°C/sec
<b>Step 3</b>	Begin Loop for 60 Iterations	-
<b>Step 3.1</b>	Temperature 95°C for 15 seconds	2°C/sec
<b>Step 3.2</b>	Temperature 62°C for 60 seconds	2°C/sec
<b>Step 4</b>	Temperature 58°C for 300 seconds	1°C/sec
<b>Step 5</b>	Release for Ruby Chip	-

## Image Acquisition

Download the dedicated scanning file from the Technical Resources section of the Stilla Technologies website:

- ScanningTemplate\_Prism6\_TERT\_R51024.ncx (6-color naica® system)
- NioProtocol\_6C-60X-62°C-60s.nioprotocol (Nio™ Digital PCR)
- NioAssay\_6C\_TERT\_R51024.nioassay (Nio™ Digital PCR)

## Image Analysis

The following files are embedded in the dedicated scanning files listed above:

- CompensationMatrix\_Prism6\_TERT\_R51024.ncm (6-color naica® system)
- CompensationMatrix\_Nio\_TERT\_R51024.ncm (Nio™ Digital PCR)
- AnalysisConfiguration\_TERT\_R51024.nca (all systems)

## Consumables Required but Not Provided

- Ruby Chip (C16011)
- naica® PCR MIX 10X (R10106)
- Universal Reporters 7 (R42401 200 reactions, R42402 1000 reactions)
- Nuclease-free water
- DMSO (Sigma-Aldrich Reference: D8418)
- 7-deaza-dGTP (Roche, Sigma-Aldrich Reference: 10988537001)

## Instruction for PCR Mix Preparation

To ensure good assay performance, two enhancers must be added to the PCR mix: DMSO (4% vol./vol.) and 7-deaza-dGTP (200 µM). Specific instructions for preparing the PCR mix are given below.

Reagent Name	Initial Concentration	Final Concentration	Volume per reaction (µL)
naica® PCR MIX Buffer A ●	10x	1x	0.60
naica® PCR MIX Buffer B ●	100%	4%	0.24
Crystal Flex Probes ●	10x	1x	0.60
Crystal Universal Reporter Tube A ●	40x	1x	0.15
Crystal Universal Reporter Tube B ●	40x	1x	0.15
DMSO	100%	4%	0.24
7-deaza-dGTP	10mM	0.2mM	0.12
Nuclease-free water	NA	NA	Variable
<b>Template DNA</b>	<b>NA</b>	<b>NA</b>	<b>Variable</b>
<i>or Positive Control</i> ○	10x	1x	0.60
<i>Total reaction volume (µL)</i>			<i>6.0</i>

## Representative Data and Instructions for Analysis

Set thresholds for separating positive and negative populations on the 1D plots. To optimize the analysis, the thresholds should be set at approximately equal distance from the positive and negative clusters. Examples of results obtained on the Nio™+ system are given below.

Wet lab testing was carried out using genomic hgDNA and H<sub>2</sub>O as negative controls and a positive control consisting of hgDNA and 3 synthetic TERT mutants (C228T, C242T-C243T, C250T). Synthetic TERT mutants were also tested individually (C228T, C242T-C243T, C250T).

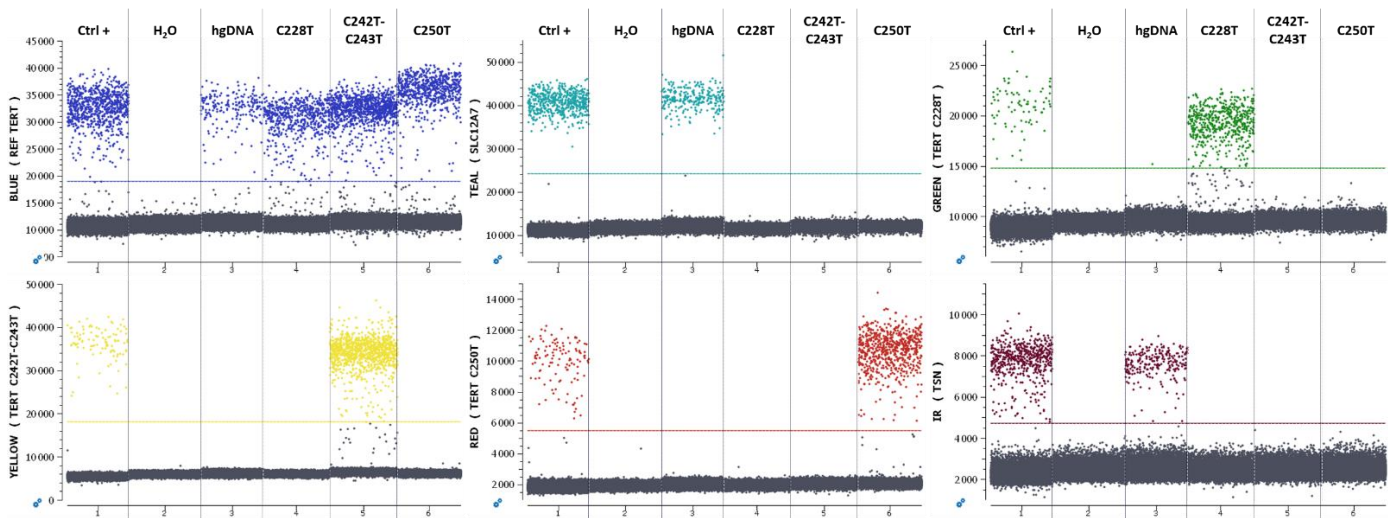


Figure 1: 1D plots obtained during wet lab testing on the Nio™+. The thresholds are set at approximately equal distance from the positive and negative clusters.



Stilla Technologies  
 F-94800 Villejuif, FRANCE

Registered names and trademarks used in this document, even when not specifically marked, are not to be considered unprotected by law.